


## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<b>(51) International Patent Classification <sup>6</sup> :</b> <b>A61L 2/00</b>	<b>A2</b>	<b>(11) International Publication Number:</b> <b>WO 98/30249</b>
		<b>(43) International Publication Date:</b> 16 July 1998 (16.07.98)
<b>(21) International Application Number:</b> PCT/US98/00635		<b>(81) Designated States:</b> AU, CA, JP, KR, SG, European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).
<b>(22) International Filing Date:</b> 13 January 1998 (13.01.98)		
<b>(30) Priority Data:</b> 08/782,647                      14 January 1997 (14.01.97)                      US		
<b>(71) Applicant:</b> STERIS CORPORATION [US/US]; 5960 Heisley Road, Mentor, OH 44060 (US).		
<b>(72) Inventors:</b> HAIRE, Donna, M.; 5273 E. 117th Street, Garfield Heights, OH 44125 (US). WOLF-BLOOM, David, F.; Apartment 203, 2540 North Moreland Boulevard, Shaker Heights, OH 44120 (US). MALCHESKY, Paul, S.; 239 Barrington Ridge, Painesville Twp., OH 44077 (US).		
<b>(74) Agent:</b> KOCOVSKY, Thomas, E., Jr.; Fay, Sharpe, Beall, Fagan, Minnich & McKee, Suite 700, 1100 Superior Avenue, Cleveland, OH 44114-2518 (US).		<b>Published</b> <i>Without international search report and to be republished upon receipt of that report.</i>

(54) Title: METHOD AND APPARATUS FOR CLEANING, DECONTAMINATING, AND STERILIZING CATHETERS

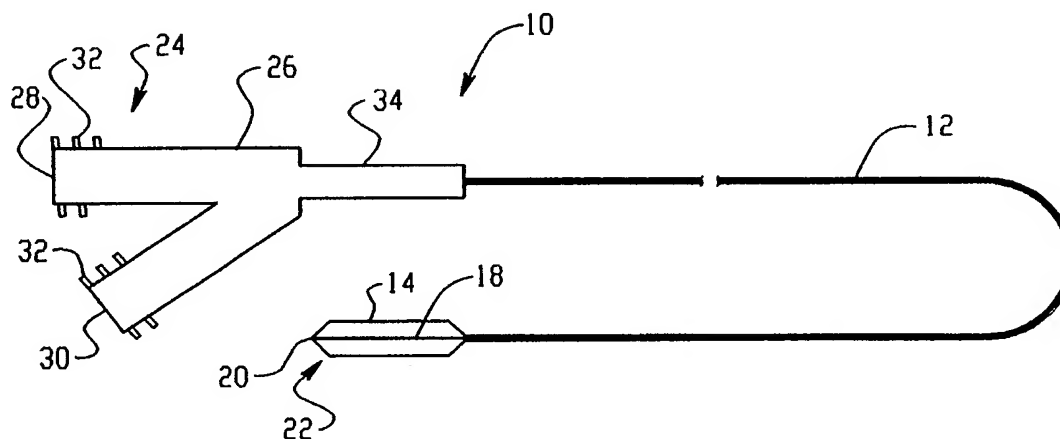

## (57) Abstract

A method for cleaning, decontaminating, and sterilizing catheters (10) using a combination of liquid and gaseous/plasma sterilization techniques to ensure the complete and efficient sterilization of a catheter (10). Angiographic dye and saline are removed from the interior (36) of the balloon (14) and its lumen (16). The outer surfaces of the catheter (10) and a guide wire lumen (18) of the catheter (10) are cleaned, decontaminated, and sterilized (42) with a liquid sterilant. The liquid sterilant fills a balloon (14) and a balloon lumen (16) of the catheter (10). The liquid sterilant is retained in the balloon (14) and the lumen (16) for a selected amount of time. Thereafter, the liquid sterilant is drained from the balloon (14) and the balloon lumen (16). The filling, retaining, and draining steps are repeated until an interior (36) of the balloon (14) and the balloon lumen (16) are sterilized. Residual liquid sterilant is rinsed from the interior (36) of the balloon (14) and the balloon lumen (16). The catheter (10) is dried and then a plasma or gaseous sterilant is used to sterilize at least the outer surfaces and the guide wire lumen (18) of the catheter (10).

***FOR THE PURPOSES OF INFORMATION ONLY***

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

- 1 -

**Method and Apparatus for Cleaning,  
Decontaminating, and Sterilizing Catheters**

**Background of the Invention**

The present invention relates to the art of cleaning, decontaminating, and sterilizing medical instruments and devices. It finds particular application  
5 in conjunction with the cleaning, decontamination, and sterilization of previously used catheters, such as percutaneous transluminal coronary angioplasty catheters (PTCA catheters), for subsequent reuse and will be described with particular reference thereto.

10 As the costs associated with the delivery of effective healthcare continue to rise, there is a continuing effort on the part of doctors, healthcare facilities, and insurers to find ways of reducing these costs. The increasing popularity of single-use  
15 disposable medical devices has contributed to the increasing costs of surgery. The PTCA catheter is a widely used single-use disposable medical device used by surgeons to perform percutaneous transluminal angioplasty, a surgical procedure to clear blockages of  
20 plaque and the like from the arteries of a patient.

A percutaneous transluminal coronary angioplasty is carried out utilizing a PTCA catheter which typically takes the form of a balloon and a balloon lumen having a coaxial guide wire lumen passing  
25 therethrough. The proximal end of the PTCA catheter is bifurcated and includes a guide wire lumen port providing access to the guide wire lumen and a balloon lumen port providing access to the balloon lumen, and thus, the balloon. The distal end of the PTCA catheter includes  
30 the closed balloon which is sealed around the open end of

- 2 -

the guide wire lumen, i.e., the guide wire lumen passes through the balloon and is open at its distal end. The surgeon uses a guide wire to guide the PTCA catheter into the vascular system of the patient to an area where a  
5 blockage exists. The catheter is often inserted into the femoral artery of the patient, and therefore, the catheter must be of a significant length (often 150 centimeters) to reach areas near the patient's heart.

After the catheter is in position, the surgeon  
10 inflates the balloon with a fluid, such as saline, by injecting the saline into the balloon lumen port of the catheter. Often, the saline includes a radiographic dye which enables the position and the inflated profile of the balloon to be monitored radiographically. The  
15 balloon expands radially and thus forces the arterial plaque radially outward into the wall of the artery. The surgeon then deflates the balloon, withdraws the catheter from the patient's vascular system, and disposes of the catheter.

20 Usually, more than one catheter is used on a particular patient, at a cost of several hundred dollars or more per catheter. Thus, a significant cost savings could be realized from the reuse of PTCA catheters. One difficulty associated with cleaning and sterilizing  
25 catheters such as PTCA catheters is attributable to a combination of the length of the catheter, the narrowness of the catheter and the guide wire and balloon lumens, and the closed balloon at the distal end of the catheter which does not allow liquid sterilant to be flushed  
30 through the balloon lumen and the balloon.

The cleaning of these devices by hand is time consuming and unreliable. Prior attempts to automate the process have resulted in unduly complex systems that have

- 3 -

not been proven to be effective. Prior systems rely solely on liquid sterilization and are not compatible with gas sterilization techniques such as the use of ethylene oxide gas (EO) and these prior systems specifically teach away from the use of EO. Even with respect to the liquid sterilization utilized in the prior systems, the methods and apparatus disclosed do not control the "contact time" of the cleaning agent and the sterilant within the balloon and balloon lumen. They require the balloon to be pressurized with liquid sterilant and a cleaning agent an excessive number of times, reducing the remaining useful life of the balloon. Furthermore, merely filling the balloon lumen and balloon with a cleaning agent and sterilant and immediately flushing the same therefrom a selected amount of times, without further controls, has been found to be an ineffective cleaning and sterilization technique in certain circumstances.

One prior PTCA catheter sterilization method requires the liquid sterilized catheter to be rinsed of liquid sterilant immediately prior to use. This prior method requires a nurse or a surgical assistant to rinse the balloon and balloon lumen by injecting several syringes or more of sterile saline into the balloon. The saline that drains from the balloon and balloon lumen must be tested for the presence of sterilant using chemical test strips. The rinsing must be continued in this manner until the test strips indicate that the concentration of sterilant in the evacuated rinse fluid is below safe thresholds. It can be seen that the foregoing PTCA catheter sterilization method is time consuming and inconvenient. Also, the rinsing of the catheter just prior to its use results in a wet catheter

- 4 -

being presented to the surgeon, which some surgeons may find objectionable.

Another disadvantage of known catheter sterilization systems is their requirement that a single  
5 catheter be processed or sterilized and stored in a specially designed cassette while awaiting use. These cassettes must be specially pressurized and capped in order for them to maintain the sterility of the catheter. Also, each cassette holds only one catheter, and thus,  
10 the efficiency of this prior system is necessarily limited.

The present invention provides a new and improved catheter cleaning, decontamination, and sterilization method and apparatus which overcomes the  
15 above-referenced problems and others.

#### Summary of the Invention

In accordance with one aspect of the present invention, a method of cleaning, decontaminating, and  
20 sterilizing an elongated catheter having outer surfaces, a balloon, and a dead-end balloon lumen open at a first end and closed by the balloon at a second end is provided. Using a liquid decontaminant, the outer surfaces of the catheter are cleaned and decontaminated.  
25 The balloon lumen and the interior of the balloon are cleaned, decontaminated, and sterilized with a liquid sterilant. The catheter is dried and thereafter, at least the outer surfaces of the catheter are sterilized with a gaseous or plasma sterilant.

30 In accordance with a more limited aspect of the present invention, the step of sterilizing the balloon lumen and the interior of the balloon of the catheter includes rinsing the dye and saline from within the

- 5 -

balloon and the balloon lumen. Liquid sterilant is communicated into the interior of the balloon and into the balloon lumen and retained in the balloon and balloon lumen for a selected amount of time. The liquid  
5 sterilant is then drained from the balloon and balloon lumen of the catheter. The filling, retention, and draining steps are repeated until the interior of the balloon and the balloon lumen are sterilized.

In accordance with yet another aspect of the  
10 present invention, an apparatus for cleaning, decontaminating, and sterilizing at least the balloon lumen and the interior of the balloon of a plurality of catheters using the method of the present invention is provided. The apparatus includes a supply of liquid  
15 sterilant and a liquid bath for receiving a plurality of catheters therein to maintain the catheters at a selected temperature. A manifold is in selective fluid communication with the liquid sterilant supply and includes a plurality of catheter connection fittings for  
20 connecting the balloon lumen of each of the plurality of catheters in fluid communication with the manifold. A pump pumps liquid sterilant under pressure from the supply of liquid sterilant into the balloon lumen and balloon of each of the plurality of catheters connected  
25 to the manifold and also evacuates the liquid sterilant from the balloon and the balloon lumen of each of the plurality of catheters. At least one valve selectively blocks the flow of liquid sterilant to and from the manifold. An electronic controller is connected to the  
30 pump and the at least one valve for controlling the operation of the pump and the at least one valve. The controller is programmed to control the pump and the at least one valve to repeat the operations of operating the

- 6 -

pump to fill the balloon and balloon lumen of each of the plurality of catheters connected to the manifold with liquid sterilant; closing the at least one valve to retain the liquid sterilant within the balloon lumen and  
5 balloon of each of the plurality of catheters connected to the manifold for a selected amount of time; and, opening the at least one valve and operating the pump to evacuate essentially all of the liquid sterilant from within the balloon and balloon lumen of each of the  
10 plurality of catheters connected to the manifold.

One advantage of the present invention is the more effective cleaning and sterilization of catheters.

Another advantage of the present invention is the efficiency and ease with which catheters are  
15 sterilized.

Another advantage of the present invention is the combination of liquid and gas or plasma sterilization techniques to effectively sterilize catheters.

Another advantage of the present invention is the  
20 elimination of the need to sterilize and store the catheters in special pressurized containers.

Another advantage of the present invention is that the sterilized catheters are rinsed, dried, and ready for immediate use without further rinsing or  
25 preparation.

Another advantage of the present invention is the ability to simultaneously sterilize the interior of the balloon and the balloon lumen of each of a plurality of catheters.

30 Still further advantages of the present invention will become apparent to those of ordinary skill in the art upon reading and understanding the following detailed description of the preferred embodiments.



- 7 -

**Brief Description of the Drawings**

The invention may take form in various components and arrangements of components, and in various steps and arrangements of steps. The drawings are only for purposes of illustrating a preferred embodiment and are not to be construed as limiting the invention.

FIGURE 1A shows a PTCA catheter suitable for being sterilized in accordance with the method and apparatus of the present invention;

FIGURE 1B is a partial enlarged diagrammatic illustration of distal portion of the PTCA catheter of FIG. 1, including the balloon, balloon lumen, and guide wire lumen thereof;

FIGURE 2 is a flow chart illustrating catheter cleaning and sterilization in accordance with the present invention;

FIGURE 3 is a flow chart illustrating removing the catheter from the patient and preserving the catheter for sterilization in accordance with the present invention;

FIGURE 4 is a flow chart illustrating performing the first cleaning and decontamination of the catheter;

FIGURE 5 is a flow chart illustrating cleaning, decontaminating, and sterilizing the balloon lumen and interior of the balloon;

FIGURE 6 is a flow chart illustrating the gaseous or plasma sterilization of the catheter;

FIGURE 7 is a schematic view of a balloon and balloon lumen pump system as it is configured for liquid sterilization of the balloon and balloon lumen; and

- 8 -

FIGURE 8 is a schematic view of a balloon and balloon lumen pump system as it is configured for rinsing the balloon and balloon lumen.

5     **Detailed Description of the Preferred Embodiments**

With reference to FIGURES 1A and 1B, a percutaneous transluminal coronary angioplasty (PTCA) catheter **10** includes an elongated and flexible tubular member **12** with a balloon **14** located at the distal end. As is seen most clearly in FIGURE 1A, the tubular member **12** provides a channel or lumen **16** to the balloon **14**. A through-lumen, referred to as a guide wire lumen **18**, is coaxially positioned within balloon lumen **16** and extends through balloon **14** to an open distal end **20**. The balloon **14** is closed at its distal end **22** around the guide wire lumen **18**.

The tubular member **12** of the catheter **10** has a proximal end **24** including a bifurcated hub **26**. The bifurcated hub **26** includes a guide wire lumen access port **28** providing access to the guide wire lumen **18** and a balloon lumen access port **30** providing access to the balloon lumen **16**, and thus to the balloon **14**. Each port **28**, **30** typically includes commonly known luer lock connectors **32** or the equivalent. As shown herein, the bifurcated hub **26** is connected to the tubular member **12** through a strain relief sheath **34** for a more durable interconnection. The illustrated PTCA catheter **10** is an example of a catheter that can be cleaned, decontaminated, and sterilized utilizing a method and apparatus in accordance with the present invention. Those skilled in the art will recognize that the PTCA catheter **10** may be modified but will remain suitable for

- 9 -

sterilization in accordance with the present invention, and that a sterilization method and apparatus in accordance with the present invention may be utilized to clean and sterilize other catheters having a balloon and  
5 balloon lumen as described above.

During angioplasty procedures, the tubular member **12** of the catheter **10** is inserted into the vascular system of the patient, and thus, the outer surfaces of the catheter **10**, including the outer surfaces  
10 of the hub **26**, the strain relief sheath **34**, the tubular member **12**, and the balloon **14** become contaminated with the blood and other bodily fluids of the angioplasty patient. Furthermore, the guide wire lumen **18**, which is open at the distal end **20**, also becomes contaminated with  
15 the patient's blood. In most angioplasty procedures, the balloon lumen **16** and the interior **36** of the balloon **14** will not become contaminated with the patient's bodily fluids. In subsequent angioplasty procedures, any contamination within the balloon **14** would not be readily  
20 transmissible into the blood of the later patient in light of the closed nature of the balloon. However, the balloon **14** may burst upon inflation in a later procedure, and for this and other reasons, the safe sterilization of PTCA catheters **10** includes a complete sterilization of  
25 the balloon lumen **16** and the interior **36** of the balloon **14**.

Furthermore, during angioplasty procedures, an angiographic dye and saline mixture is communicated into the interior **36** of the balloon **14**. This dye and saline  
30 mixture are removed from the interior **36** of the balloon **14** within a relatively short time (less than 24 hours) lest it crystallizes, adversely affecting the utility of

- 10 -

the catheter **10** for subsequent angioplasty procedures. The method and apparatus of the present invention result in the sterilization of an entire PTCA catheter **10**, including all of the outer surfaces, as well as the guide  
5 wire lumen **18**, the balloon lumen **16**, and the interior **36** of the balloon **14**.

With reference to FIGURE 2, the preferred overall method of sterilizing a PTCA catheter **10** is shown. Each step or means shown in FIGURE 2 is described  
10 in further detail with reference to FIGURES 3 - 6. In a step **40** the catheter **10** is recovered from the patient and preserved for sterilization. Once the catheter **10** has been recovered and preserved for later sterilization, a step or means **42** cleans and decontaminates the outer  
15 surfaces and the guide wire lumen **18** of the catheter **10**. Following the cleaning and decontamination of the outer surfaces and the guide wire lumen **18** of the catheter **10**, a step or means **44** cleans, decontaminates, and sterilizes the balloon lumen **16** and the interior **36** of the balloon  
20 **14** of the catheter **10**. Preferably, a step or means **46** provides a second cleaning and decontamination of the outer surfaces and the guide wire lumen **18** of the catheter **10**. A step or means **48** dries the catheter **10**, and a step or means **50** sterilizes the catheter with a  
25 gaseous sterilant, resulting in a completely sterilized catheter that is free of harmful amounts of residual sterilant, dry, and ready for reuse.

With reference to FIGURE 3, the step **40** of recovering the catheter **10** from the patient is shown in  
30 greater detail and includes steps or means **40a** - **40d**. In a step **40a**, the catheter **10** is removed from the patient. This step is generally performed manually. Immediately

- 11 -

following the removal of the catheter **10** from the patient, a step or means **40b** fills the balloon **14** of the catheter **10** with a sterile liquid, such as sterile saline, sterile water, or the like, and caps the balloon  
5 lumen port **30** of the catheter **10** to retain the sterile liquid in the balloon **14** and balloon lumen **16**. The sterile liquid in the balloon **14** and balloon lumen **16** and the capping of the lumen port **30** prevents the angiographic dye and saline within the balloon **14** from  
10 crystallizing. Furthermore, capping the balloon lumen port **30** not only prevents the escape of the sterile fluid from the balloon **14**, but also prevents the contamination of the interior **36** of the balloon **14** with blood and other  
contaminates that are in the guide wire lumen **18** and on  
15 the outer surfaces of the catheter **10**.

A step or means **40c** flushes the guide wire lumen **18** with a liquid and a step or means **40d** submerges or otherwise surrounds the catheter **10** with a liquid. Although ordinary saline or the like may be utilized as  
20 the liquid in the step or means **40c** and the step or means **40d**, the liquid utilized is preferably an anticoagulant liquid solution. One suitable solution used in the steps or means **40c** and **40d** is a solution of 10,000 units of Heparin per 1000 milliliters (ml.) of saline. With such  
25 a solution, the guide wire lumen **18** of the catheter **10** is flushed with approximately 10 ml. of the solution and the catheter is then submerged in the solution for about approximately 15 minutes. The anticoagulant solution rinses blood and the like from the outer surfaces of the  
30 catheter **10** and from within the guide wire lumen **18**. It also prevents the clotting and hardening of the blood on the catheter **10** and in the guide wire lumen **18**. Those

- 12 -

skilled in the art will recognize that the capped balloon lumen port **30** prevents the contamination of the interior **36** of the balloon **14** with blood when the catheter **10** is treated with the anticoagulant solution. Once the  
5 catheter **10** has been recovered from the patient and treated as described, an indefinite amount of time may pass. The catheter **10** can remain submerged in a bath of liquid as described. In practice, the catheter sterilization process continues relatively quickly  
10 following the recovery of the catheter **10** from the patient.

With reference to FIGURE 4, the sterilization process continues with the step or means **42** cleaning and decontaminating the outer surfaces and the guide wire  
15 lumen **18** of the catheter **10**. The balloon lumen port **30** remains capped at this point in the sterilization process. A step or means **42a** removes the catheter **10** from the anticoagulant liquid and a step or means **42b** surrounds the catheter **10** with liquid sterilant,  
20 decontaminant, or disinfectant and flushes the guide wire lumen **18** with liquid sterilant, decontaminant, or disinfectant for a selected amount of time.

Thereafter, a step or means **42c** rinses the outer surfaces and the guide wire lumen **18** of the  
25 catheter **10** with a sterile rinse liquid such as sterile water. While the step or means **42** decontaminates the outer surfaces of catheter **10** and also facilitates the decontamination of the guide wire lumen **18**, additional steps are provided as described below to ensure the  
30 decontamination of these areas of catheter **10**. A preferred apparatus for rinsing and decontaminating the interior surfaces of the catheter **10** is illustrated in

- 13 -

U.S. Patent Nos. 4,731,222, 4,892,706, 5,116,575, and 5,217,698 of an assignee herein.

The process either continues immediately with the step or means **44** to sterilize the balloon lumen **16** and the interior **36** of the balloon **14** or a step or means **42d** places the catheter **10** in a suitable temporary storage container, such as a sealable biohazard bag, for later processing. The step or means **42d** is utilized when further processing is conducted at a different site. Also, a hospital may wish to accumulate a large number of catheters for subsequent processing in a batch as is described below.

As is shown in detail in FIGURE 5, the reprocessing continues with the step or means **44** to clean, decontaminate, and sterilize the balloon lumen **16** and the interior **36** of the balloon **14**. A step or means **44a** uncaps the balloon lumen port **30** and withdraws the sterile fluid and any air from the balloon **14** and balloon lumen **16**. Because the angiographic dye and saline communicated into the interior **36** of the balloon **14** and the balloon lumen **16** during the angioplasty procedure can interfere with the biocidal action of the liquid sterilant and the further use of the catheter **10**, the sterilization of the balloon **14** and the balloon lumen **16** involves the removal of the dye and saline. A step or means **44b** fills the balloon **14** and the balloon lumen **16** with a sterile rinse liquid, such as sterile water. The sterile water may optionally be retained within the balloon **14** and the lumen **16** for a selected "contact time" to facilitate the rinsing process. A step or means **44c** evacuates the sterile rinse fluid from the balloon **14** and the balloon lumen **16** and a step or means **44d** repeats the

- 14 -

filling and evacuating steps **44b**, **44c** until the dye and saline are removed from the balloon **14** and the balloon lumen **16**. It has been found that repeating the steps **44b**, **44c** at least fifteen and preferably twenty times, 5 with an optional contact time of approximately fifteen - thirty seconds is effective for removing the dye and saline from the interior **36** of the balloon **14** and from the balloon lumen **16**.

In order to sterilize the interior **36** of the 10 balloon **14** and the balloon lumen **16**, a liquid sterilant is fed into the balloon **14** and the balloon lumen **16**. While simply repeatedly filling the balloon **14** and the lumen **16** with liquid sterilant and immediately evacuating the same may sterilize the interior **36** of the balloon **14** 15 and the lumen **16**, it has been found that such a method does not sterilize the interior **36** of the balloon **14** and the balloon lumen **16** as effectively as repeatedly filling the balloon **14** and balloon lumen **16** with the liquid sterilant, retaining the liquid sterilant in the balloon 20 **14** and balloon lumen **16** for a selected amount of time, and thereafter evacuating the liquid sterilant from the balloon **14** and the balloon lumen **16**. This increase in "contact time" or the amount of time that the liquid sterilant is in contact with the interior **36** of the 25 balloon **14** and the balloon lumen **16** results in more effective sterilization. It has also been found that filling the balloon **14** once with liquid sterilant and holding it filled for a selected duration is less effective than filling and emptying the balloon several 30 times over the same selected duration.

Therefore, a step or means **44e** fills the



- 15 -

balloon **14** and the balloon lumen **16** with a liquid sterilant and maintains the filled state of the balloon **14** for a selected amount of time. A step or means **44f** evacuates the liquid sterilant from the balloon **14** and  
5 lumen **16** and a step or means **44g** repeats the step **44e** and the step **44f** until the interior **36** of the balloon **14** and the balloon lumen **16** are sterilized. For example, it has been found that  $10^6$  colony forming units of spores are killed or removed from the interior **36** of the balloon **14**  
10 and the balloon lumen **16** by repeating the steps **44e** and **44f** at least eight times with a contact time of at least approximately two minutes. It is preferable to repeat the steps **44e** and **44f** at least ten times using a contact time of at least approximately one and one half minutes  
15 using a 0.2% peracetic acid sterilant. By way of example, the interior **36** of a balloon **14** and a balloon lumen **16** of a catheter **10** were inoculated with  $10^6 - 10^7$  / 0.5 ml. *B. subtilis* spores using different carrier solutions of water, saline, and 10% serum / 90% saline.  
20 A 0.2% peracetic acid sterilant was utilized. Sterilization was not achieved, with the water carrier, when steps **44e** and **44f** were repeated as follows: one time with a contact time of five minutes; two times with a contact time of seven minutes; three times with a contact  
25 time of one minute; five times with a contact time of one minute; and, ten times with a contact time of 1 minute (3 out of four trials not sterile). Sterilization was achieved, with the water carrier, when steps **44e** and **44f** were repeated as follows: four times with a contact time  
30 of two minutes; twenty-two times with a contact time of 0.25 minutes; and, twenty-four times with a contact time of 0.25 minutes. Using the serum and saline carrier

- 16 -

solution which presents the most difficult sterilization situation, when steps **44e** and **44f** were repeated ten times with a contact time of at least 1.5 - 2 minutes, sterilization resulted for seven of the nine trials.

5 With the saline carrier, six trials were conducted and steps **44e** and **44f** were repeated ten times with a contact time of two minutes. All six trials resulted in sterilization.

Following the sterilization of the interior **36**

10 of the balloon **14** and the balloon lumen **16** using the liquid sterilant as described, the liquid sterilant is rinsed from the interior **36** of the balloon **14** and from the balloon lumen **16**. Rinsing the interior **36** of the balloon **14** and the balloon lumen **16** is preferably

15 accomplished by repeatedly filling the balloon **14** and the balloon lumen **16** with a sterile rinse liquid, such as sterile water, and thereafter immediately evacuating the rinse liquid from the balloon **14** and the balloon lumen **16**. A step or means **44h** fills the balloon **14** and the

20 balloon lumen **16** with a sterile rinse liquid. A step or means **44i** evacuates the sterile rinse liquid from the balloon **14** and lumen **16** after the selected amount of time has passed. A step or means **44j** causes the means **44h** and **44i** to repeat the filling and evacuating steps until the

25 amount of residual sterilant in the interior **36** of the balloon **14** and in the balloon lumen **16** is below the selected threshold.

For example, using a peracetic acid sterilant and a sterile rinse liquid of sterile deionized/filtered

30 water, it has been found that repeating steps **44h** and **44i** at least fifteen times, and preferably twenty times, results in the interior **36** of the balloon **14** and the

- 17 -

lumen **16** being essentially free of residual sterilant. Once the rinsing process is complete, a step or means **44k** evacuates the sterile rinse liquid from the balloon **14** and its lumen **16** and a step or means **44l** caps the balloon  
5 lumen port **30** to prevent recontamination.

In case of any contamination of the catheter **10** during transport or handling with respect to the above procedures, it is preferable to provide an optional step or means **46** for a second cleaning and decontamination of  
10 the outer surfaces and the guide wire lumen **18** of the catheter **10**. The step or means **46** performs substantially the same operations as the step or means **42** as described above in detail with reference to FIGURE 4. The step or means **46** ensures that the outer surfaces of the catheter  
15 **10** are decontaminated and facilitates the sterilization of the guide wire lumen **18**. Following the second cleaning and decontamination of the outer surfaces and the guide wire lumen **18** of the catheter **10** with a liquid sterilant, the catheter **10** is completely dried by a step  
20 or means **48** in preparation for a step or means **50** to gas sterilize the catheter **10**. As is shown in FIGURE 6, a step or means **48a** uncaps the balloon lumen port **30** of the catheter **10**. A step or means **48b** dries the outer surfaces, the guide wire lumen **18**, the balloon lumen **16**,  
25 and the interior **36** of the balloon **14**. The step or means **48b** is preferably carried out in a sterile vacuum oven system with -25 to -30 inches of mercury (Hg) at a temperature of 30 degrees C to 40 degrees C for 1.5 hours. Alternatively, the oven can be a non-sterile  
30 vacuum oven system.

With continuing reference to FIGURE 6, once the

- 18 -

catheter **10** is dry, the step or means **50** gas sterilizes the catheter **10**, and in particular the outer surfaces and the guide wire lumen **18** thereof, preferably using a gaseous or plasma sterilant such as ethylene oxide (EO) gas, vapor phase hydrogen peroxide, or the like. A step or means **50a** deflates the balloon **14** and places a protective sheath over the balloon **14**. A step or means **50b** places the catheter in gas sterilization packaging, such as a standard EO sterilization bag. A step or means **50c** exposes the packaged catheter **10** to a plasma or gaseous sterilant such as EO for a selected amount of time. For example, the step or means **50c** exposes the catheter **10** to 100% EO for approximately 4 to 5 hours at 90 degrees F. A 4.75 hour EO exposure time has been found to be effective. Following the exposure of the catheter **10** to EO, a step or means **50d** aerates the catheter **10** and the packaging to disperse residual gaseous sterilant. It has been found effective for the step or means **50d** to aerate the catheter **10** and the gas sterilization packaging for 12 hours at approximately 90 degrees F. The catheter **10** can then be safely reused for another angioplasty procedure with a different patient.

With reference to FIGURE 7, a supply of liquid sterilant **62** is heated in a water bath **64**. The heated water bath **64** also receives a plurality of the catheters **10** during the sterilization process. The liquid sterilant, such as the 0.2% peracetic acid, is utilized at a temperature of 40 - 60 degrees C, preferably 50 - 56 degrees C. The heated water bath **64** heats the supply of liquid sterilant **62** and the catheters **10** placed in the bath **64** to the optimum operative temperature of the selected sterilant. A manifold **66** includes a plurality

- 19 -

of catheter connection fittings **68** for fluidically connecting the balloon lumen port **30** of each of the plurality of catheters **10** to the manifold **66**.

The manifold **66** is in fluid communication with  
5 the supply of liquid sterilant **62** through a pump **70** and is also in fluid communication with a liquid sterilant disposal reservoir **72** through the pump **70**. The liquid sterilant is pumped by the pump **70** from the supply **62** into the manifold **66** as indicated by the arrows **A** and is  
10 pumped from the manifold **66** to the disposal reservoir **72** as indicated by the arrows **B**. An inlet valve **74** and an outlet valve **76** selectively block the flow of fluid to and from manifold **66**. A pressure transducer **78** monitors the pressure of the fluid in the manifold **66**. A display  
15 **80** displays process parameters and information regarding the balloon and balloon lumen sterilization process to the operator of the apparatus **60**. The parameters preferably include the date, the time, the sterilant and water bath temperatures, the number of balloon inflation  
20 cycles, the duration of each balloon inflation cycle, and the like. Also, the apparatus is preferably enclosed within a fume hood or another suitable enclosure **86** to minimize the escape of sterilant vapors into the atmosphere, and to minimize environmental contamination  
25 of the water bath **64**, the supply of sterilant **62**, and the supply of sterile rinse fluid **82** (FIGURE 8).

FIGURE 8 schematically shows a reconfiguration of the apparatus of FIGURE 7 during the rinsing steps **44b** - **44d** and **44h** - **44j** in which the angiographic dye and  
30 saline mixture, and the liquid sterilant, are respectively rinsed from the interior **36** of the balloons **14** and the balloon lumens **16** of each catheter **10**

- 20 -

connected to the fittings 68 of manifold 66. A supply of sterile rinse liquid 82 is in fluid communication with the manifold 66 through the pump 70 and the manifold 66 is also in fluid communication with the disposal reservoir 72. The sterile rinse liquid is pumped from supply 82 to manifold 66 through conduits as shown by the arrows A, and the sterile rinse liquid is pumped from the manifold 66 to the disposal reservoir 72 through conduits as indicated by the arrows B. For rinsing operations, each catheter 10 connected to the manifold 66 is preferably submerged in an ultrasonic water bath 84.

The water baths 64, 84, the pump 70, the valves 74, 76, the pressure transducer 78, and the visual display 80 are all electrically connected to an electronic controller 88 that controls the operation of each of the noted components. The electronic controller 88 controls the application of heat and ultrasonic waves to the baths 64, 84. The electronic controller 88 also selectively operates the pump 70 as required to pump sterilant and sterile rinse liquid, and monitors the fluid pressure in the manifold 66 through electrical signals received from the transducer 78. The controller 88 selectively opens and closes the valves 74, 76 to selectively block the flow of liquid sterilant and rinse liquid to and from the manifold 66 and the disposal reservoir 72, and displays process parameters and information to an operator on the display 80. An input system 90 is connected to the electronic controller 88 for operator input of data and for operator control. A printer 92 prints out the date and time, the operator, and cycle information to provide written documentation for each catheter 10. The cycle

- 21 -

information includes such information as the number of balloon inflations with the liquid sterilant, the duration of sterilant contact, the number of rinse cycles, and the like.

5           The electronic controller **88** is programmed to operate the apparatus in accordance with the step **44** as described above with reference to FIGURES 2 and 5. Through the operation of the pump **70** and the valves **74,76**, the electronic controller **88** controls the flow of  
10 liquid sterilant and rinse liquid into and out of the balloon **14** and balloon lumen **16** of each catheter **10** connected to the manifold **66** and controls the contact time of the liquid sterilant and the rinse liquid within the balloon **14** and balloon lumen **16**.

15           The invention has been described with reference to the preferred embodiments. Obviously, modifications and alterations will occur to others upon reading and understanding the preceding detailed description. It is intended that the invention be construed as including all  
20 such modifications and alterations insofar as they come within the scope of the appended claims or the equivalents thereof.

- 22 -

Having thus described the preferred embodiments, what is claimed is:

1. A method of cleaning, decontaminating, and sterilizing an elongated catheter having outer surfaces, a balloon, and a dead-end balloon lumen open at a first end and closed by said balloon at a second end which is spaced from said first end, said method characterized by:

(a) cleaning and decontaminating the outer surfaces of the catheter with a liquid decontaminant;

(b) cleaning, decontaminating, and sterilizing the balloon lumen and the interior of the balloon with a liquid sterilant;

(c) drying the catheter; and,

(d) sterilizing at least the outer surfaces of the catheter with a gaseous or plasma sterilant.

2. The method as set forth in claim 1 wherein the step (b) of sterilizing the balloon lumen and the interior of the balloon of the catheter is further characterized by:

5 (b1) rinsing the interior of the balloon and the balloon lumen with a sterile rinse liquid to rinse any dye and saline from the balloon and the balloon lumen;

(b2) communicating the liquid sterilant into  
10 the interior of the balloon and into the balloon lumen;

(b3) retaining the liquid sterilant in the balloon and balloon lumen for a selected amount of time;

(b4) draining the liquid sterilant from the balloon and the balloon lumen; and,

15 (b5) repeating steps (b2) - (b4) until the interior of the balloon and the balloon lumen are sterilized.



- 23 -

3. The method as set forth in claim 2 wherein the step (b5) is further characterized by repeating steps (b2) - (b4) at least eight times, and wherein step (b3) is further characterized by retaining the liquid sterilant in the balloon and in the balloon lumen for at least approximately two minutes.

4. The method as set forth in claim 2 wherein step (b5) is further characterized by repeating steps (b2) - (b4) at least ten times, and wherein step (b3) is further characterized by retaining the liquid sterilant in the balloon and in the balloon lumen for at least one and one half minutes.

5. The method as set forth in any of claims 1-4 wherein the catheter also includes a guide wire lumen and wherein the cleaning and decontaminating step (a) is further characterized by:

5 blocking the balloon lumen to prevent the entrance of the liquid decontaminant into the balloon lumen and the interior of the balloon;

heating a bath of the liquid decontaminant to a temperature of greater than 40 degrees C;

10 immersing the catheter in the heated bath of liquid decontaminant for a selected amount of time; and, flushing the liquid decontaminant through the guide wire lumen of the catheter for a selected amount of time.

- 24 -

6. The method as set forth in any of claims 1-5 further characterized by repeating the cleaning and decontaminating step (a) following the sterilizing step (b).

7. The method as set forth in any of claims 1-6 wherein the catheter also includes a guide wire lumen and wherein the method is further characterized by, before the cleaning and decontaminating step (a):

5 injecting a sterile fluid into the balloon and balloon lumen of the catheter;

blocking the balloon lumen of the catheter to prevent the sterile fluid from escaping the balloon and balloon lumen; and,

10 treating the outer surfaces and the guide wire lumen of the catheter with an anticoagulant solution.

8. The method as set forth in any of claims 1-7 wherein step (b) is further characterized by:

5 rinsing the balloon and balloon lumen with a sterile rinse liquid after sterilizing the balloon lumen and the interior of the balloon until the concentration of sterilant in the balloon and balloon lumen is below a predetermined threshold.

9. The method as set forth in any of claims 2-8 further characterized by, after step (b5):

(b6) communicating a sterile rinse liquid into the interior of the balloon and into the balloon lumen;

5 (b7) retaining the sterile rinse liquid in the balloon and balloon lumen for a selected amount of time;

(b8) draining the sterile rinse liquid from the balloon and the balloon lumen;

- 25 -

10 (b9) repeating steps (b6) - (b8) until the amount of sterilant remaining in the balloon and the balloon lumen is below a selected threshold.

10. An apparatus for sterilizing at least a dead-end balloon lumen and an interior of a balloon closing a distal end of said dead-end balloon lumen of each of a plurality of catheters using the method of any of claims 1-9, the apparatus characterized by:

a supply of liquid sterilant;

a liquid bath for receiving the plurality of catheters to maintain the catheters at a selected temperature;

a manifold in selective fluid communication with the liquid sterilant supply, the manifold including a plurality of catheter connection fittings for connecting the balloon lumen of each of the plurality of catheters in fluid communication with the manifold;


a pump for pumping the liquid sterilant under pressure from the liquid sterilant supply into the balloon lumen and balloon of each of the plurality of catheters connected to the manifold and for evacuating liquid sterilant from the balloon and the balloon lumen of each of the plurality of catheters;

at least one valve for selectively blocking the flow of liquid sterilant to and from the manifold; and,


an electronic controller connected to the pump and the at least one valve for controlling the operation of the pump and the at least one valve, said electronic controller programmed to control the pump and the at least one valve to repeat the operations of operating the pump to fill the balloon and balloon lumen of each of the plurality of catheters connected to the manifold with

- 26 -

liquid sterilant; closing the at least one valve to retain the liquid sterilant within the balloon lumen and balloon of each of the plurality of catheters connected to the manifold for a selected amount of time; and, opening the at least one valve and operating the pump to evacuate essentially all of the liquid sterilant from within the balloon and balloon lumen of each of the plurality of catheters connected to the manifold.

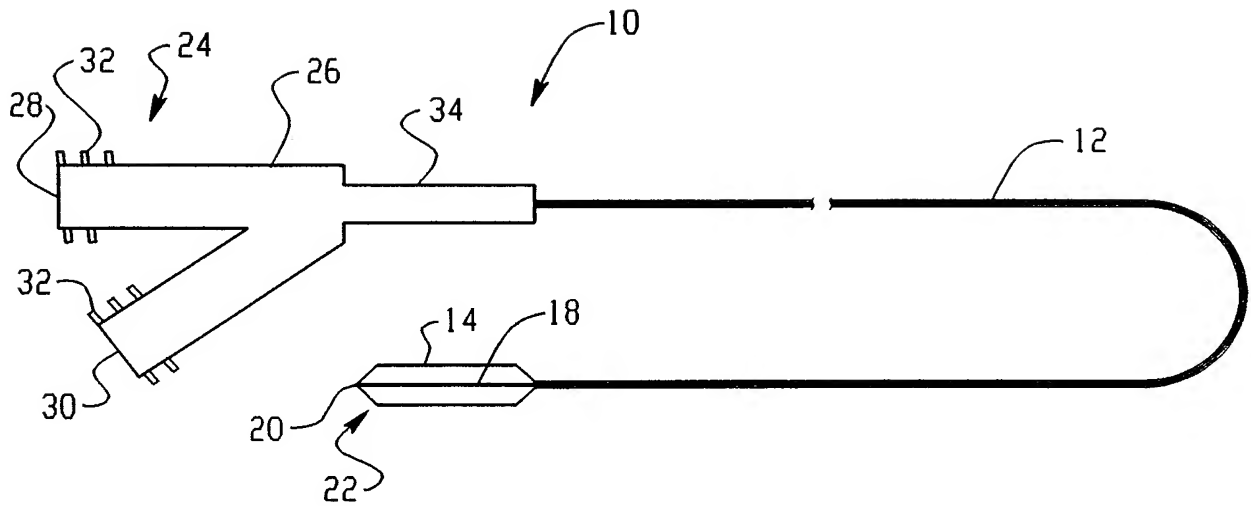


*Fig. 1A*


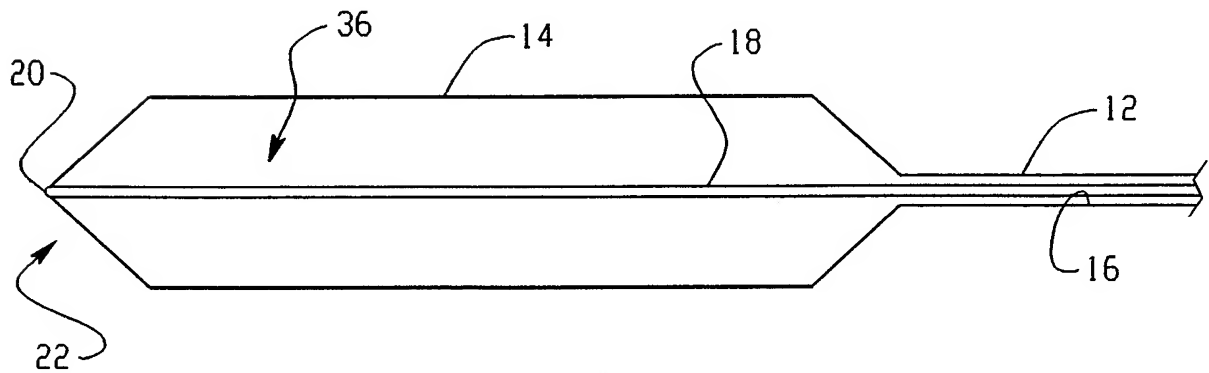


*Fig. 1B*

2/7

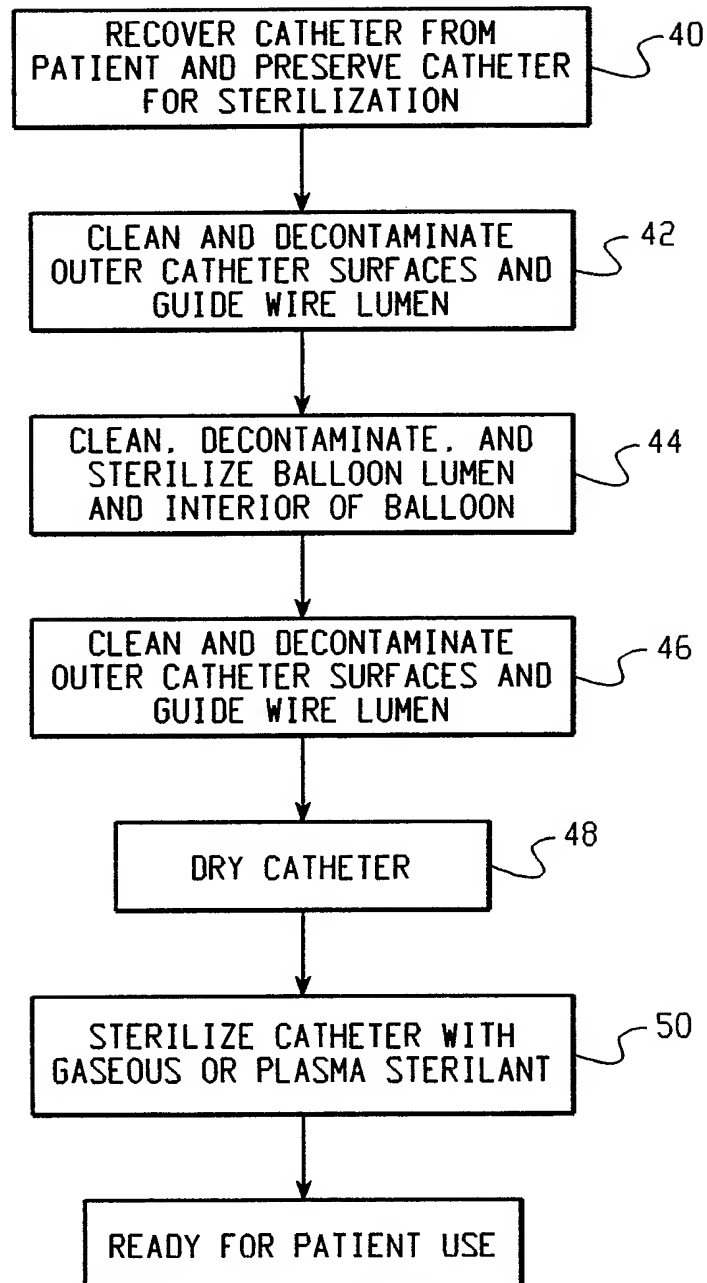*Fig. 2*

3/7

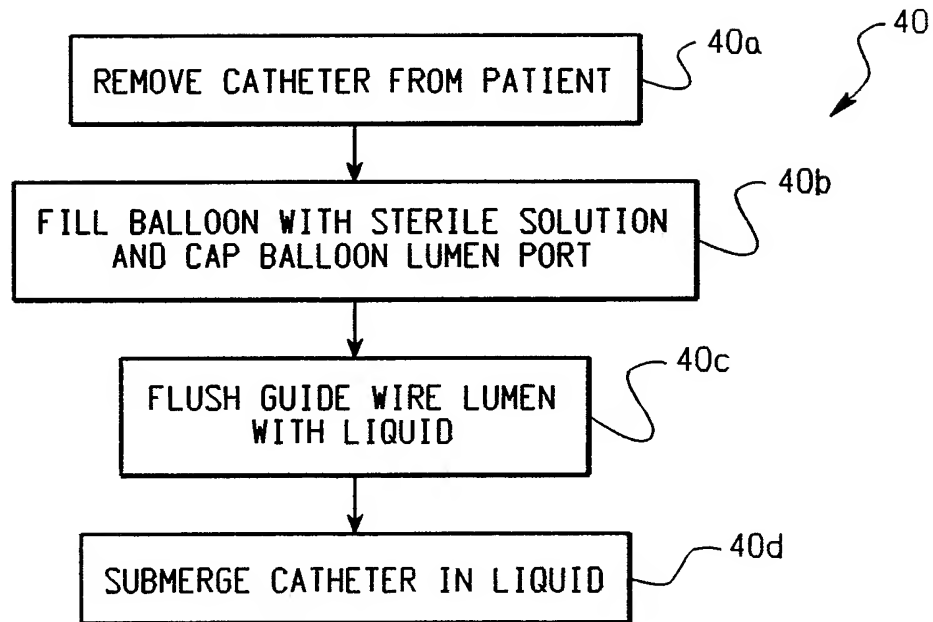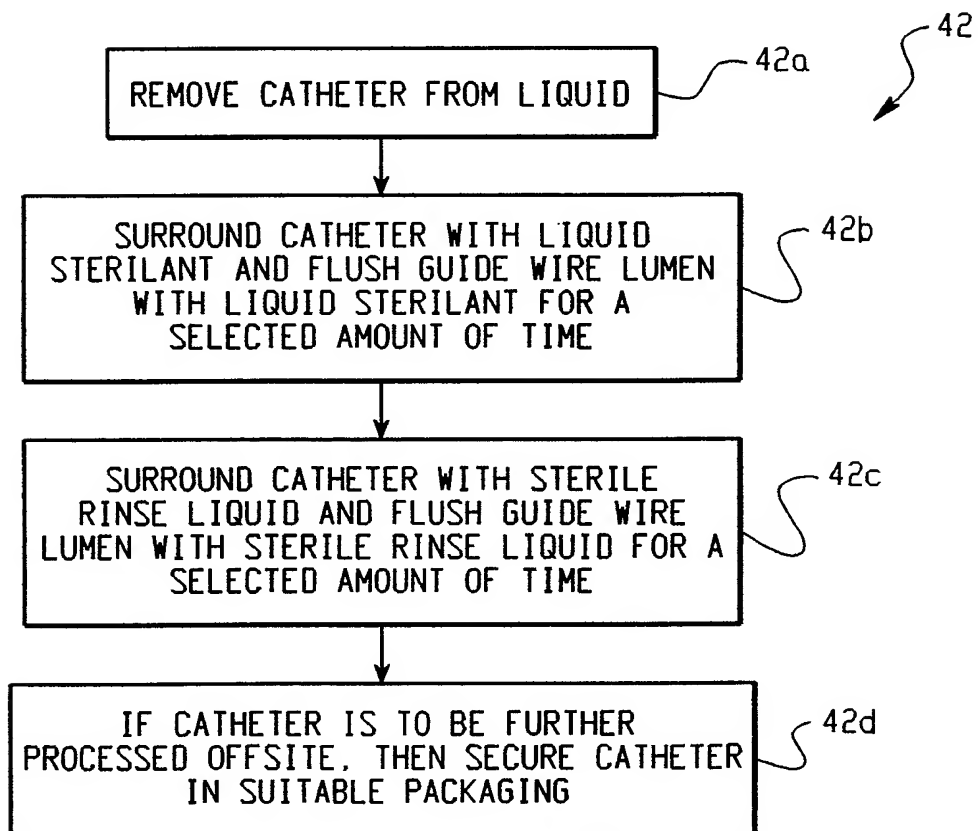*Fig. 3**Fig. 4*

4/7


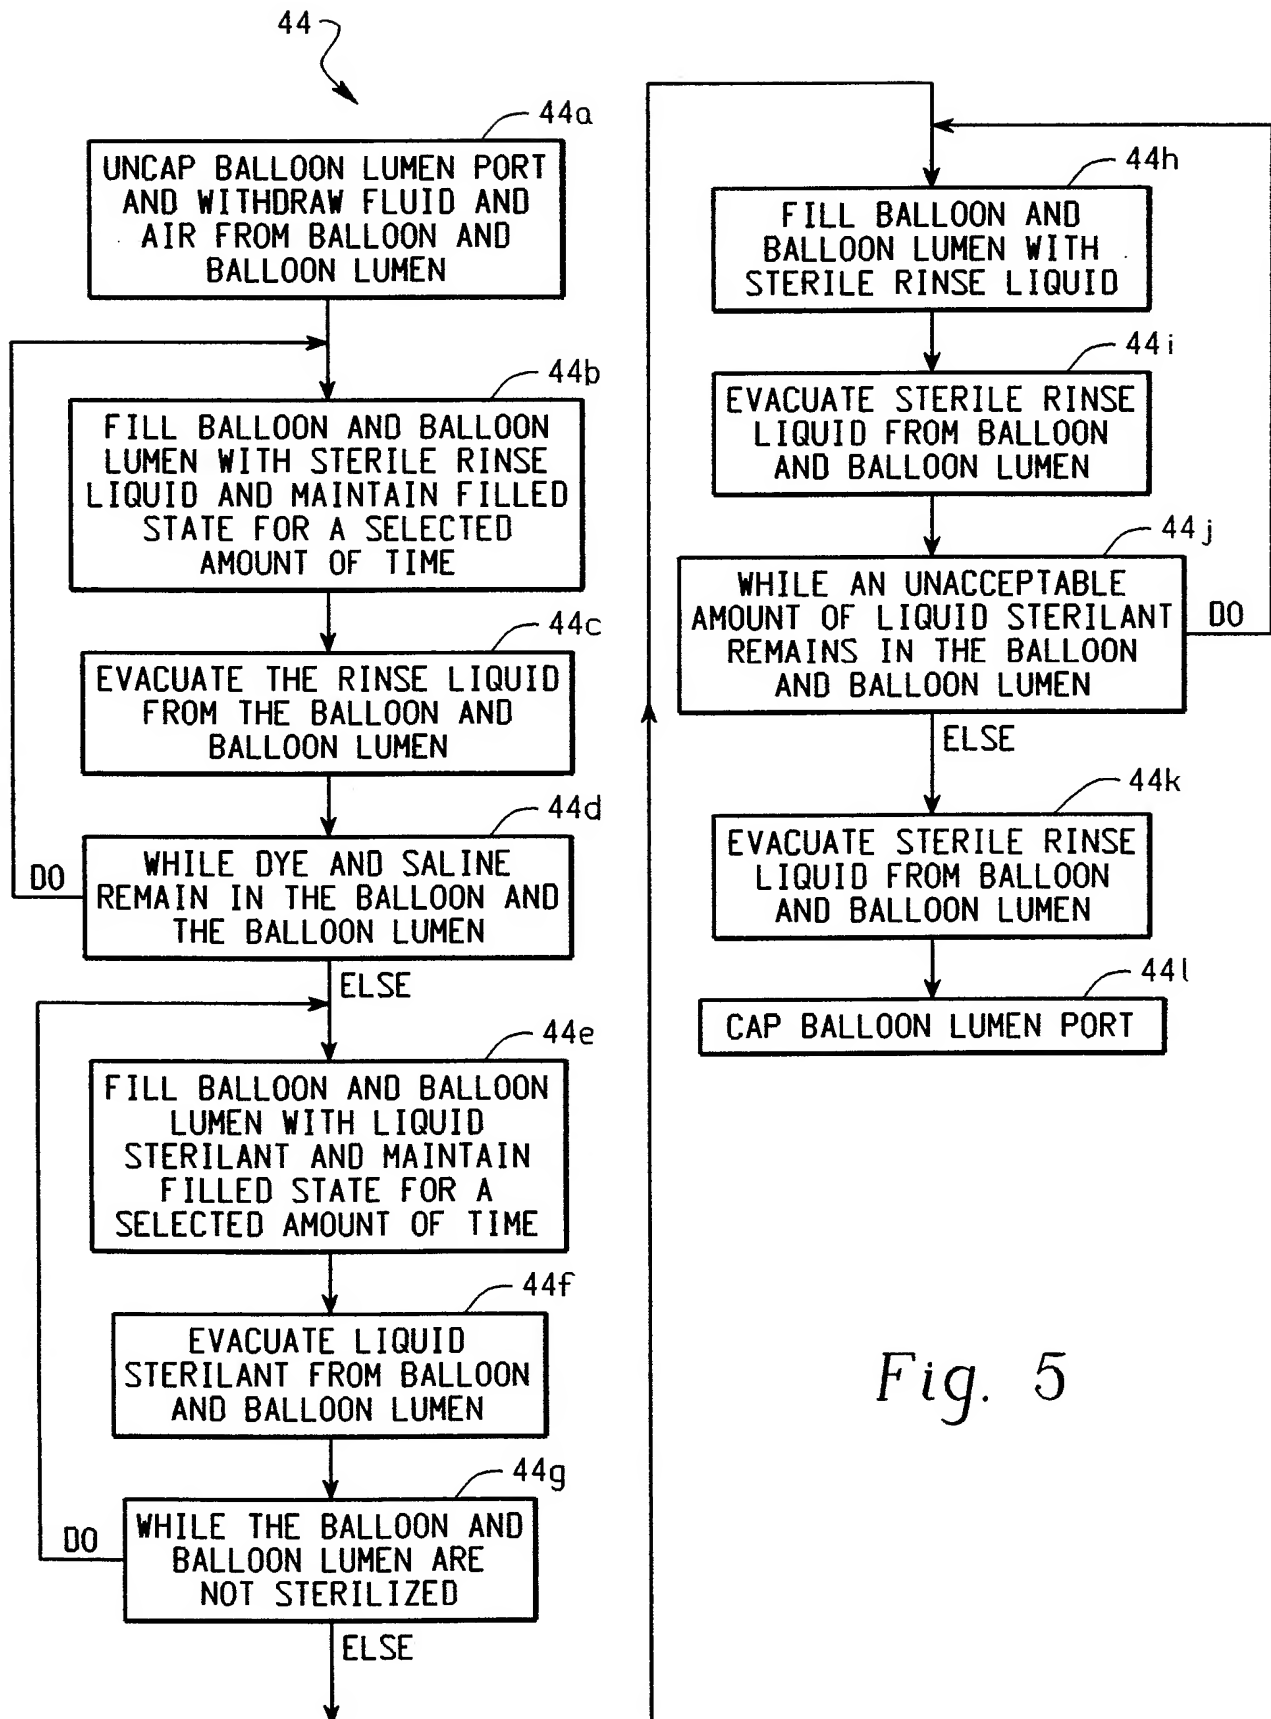


Fig. 5

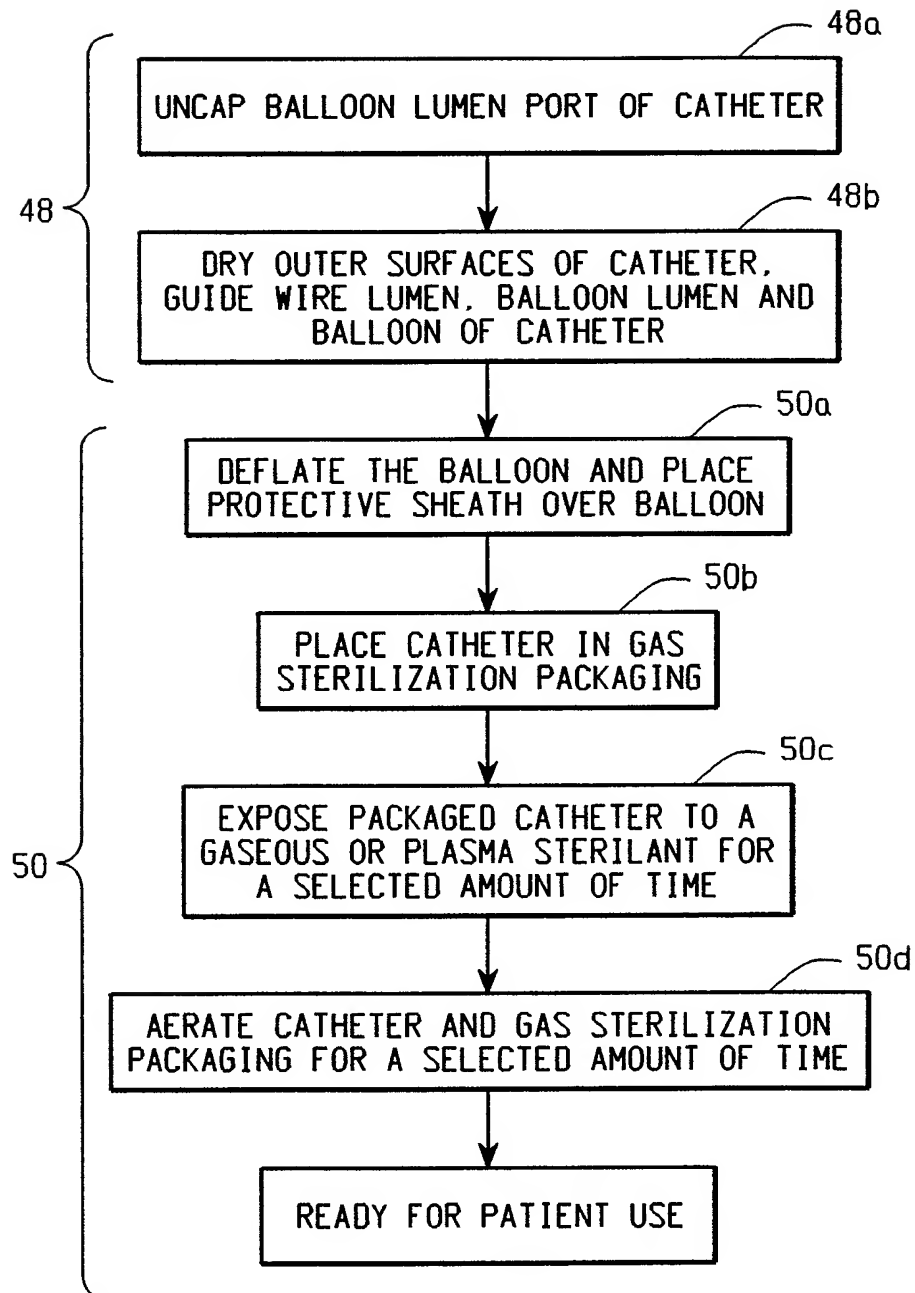

5/7

*Fig. 6*

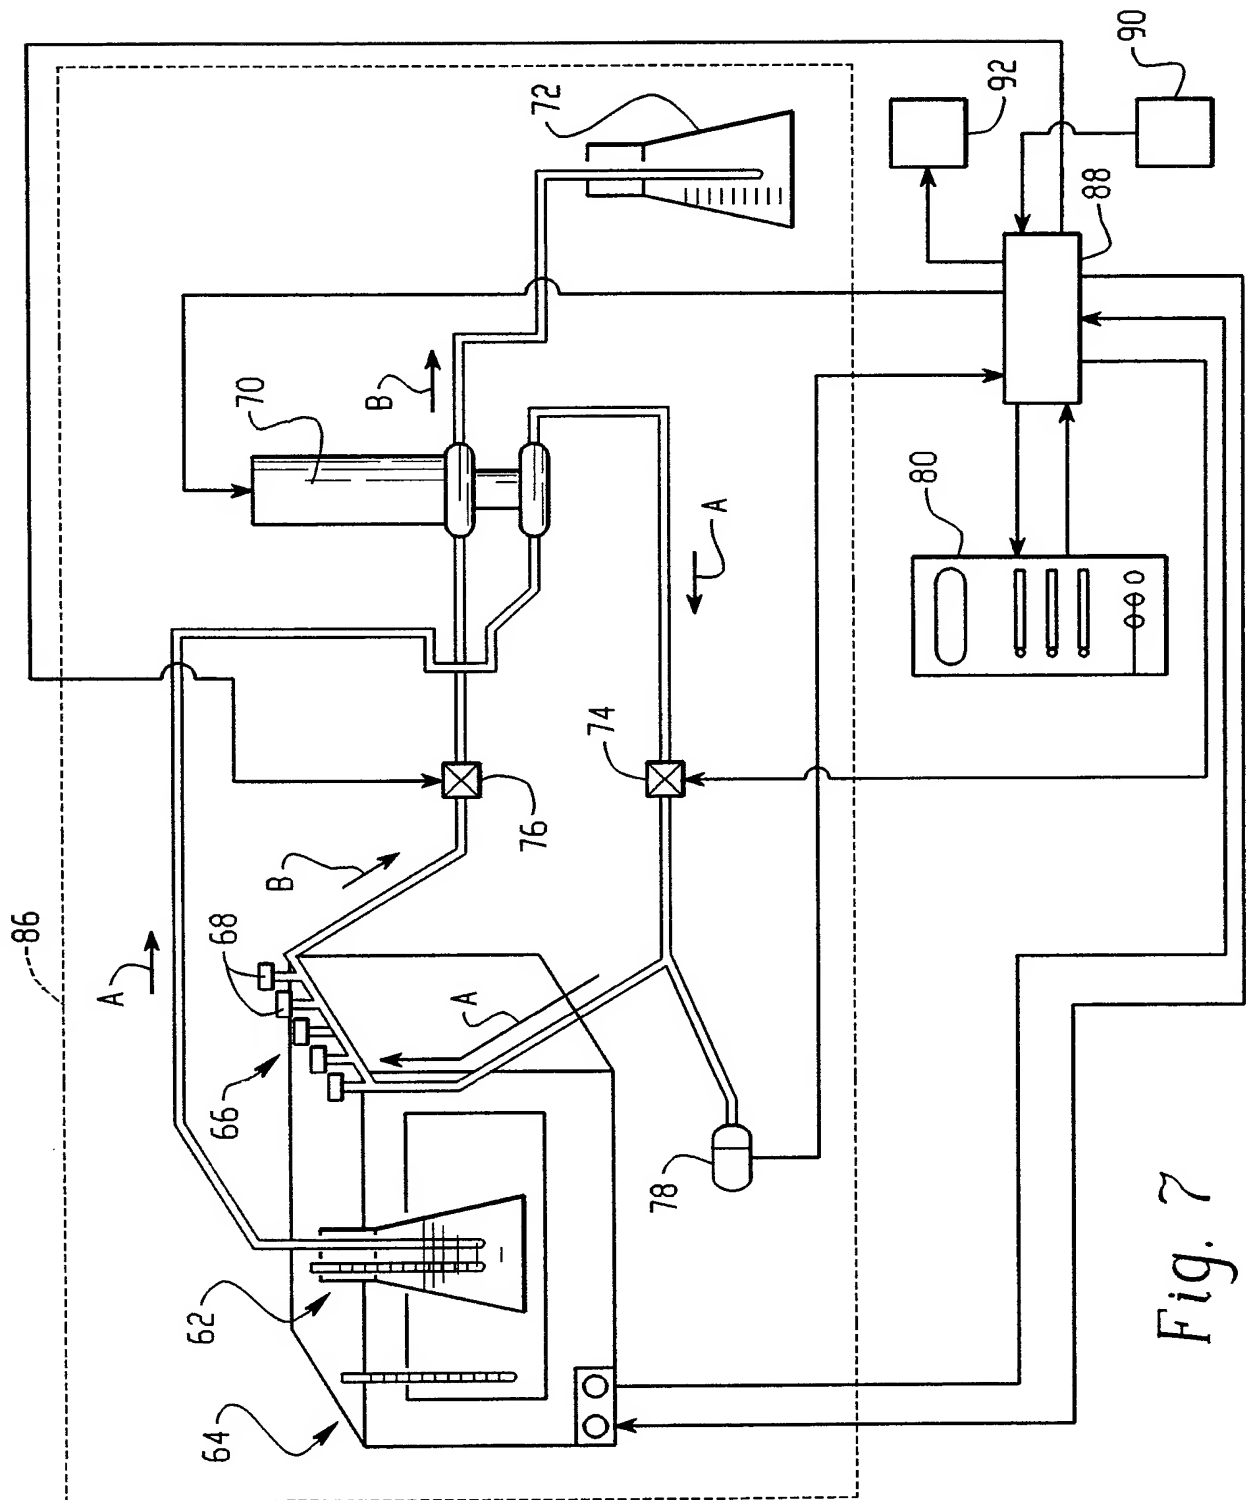


Fig. 7

